



MycoQSearchTM
***Mycoplasma* qPCR Detection Kit**

Instruction Manual

Cat. No. QD-Sample, QD -50 and QD-100

Research Use Only. Not for Use in Diagnostic Procedures.

Introduction

The *MycoQSearch* Mycoplasma qPCR Detection Kit is used to detect *Mycoplasma* infection of cell cultures by real-time quantitative PCR (qPCR) using Probe. The *MycoQSearch* Mycoplasma qPCR Detection Kit includes a Primer and Probe mixes. These mixes contain FAM labeled probe specific for mycoplasma species and Hex labeled probe for internal control DNA. The primer set is specific to the highly conserved the 16S rRNA coding region in the mycoplasma genome. This allows the detection of *M. orale*, *M. hyorhinae*, *M. arginini*, *M. fermentans*, *Acholeplasma laidlawii*, *M. hominis*, usually encountered as contaminants in cell cultures. Furthermore, this kit can detect *M. pneumoniae*, *M. salivarium*, *M. synoviae* and *Ureaplasma* species. Eukaryotic and bacterial DNA is not amplified by *MycoQsearch*TM Mycoplasma Real-Time PCR Detection Kit.

The *MycoQSearch* Mycoplasma qPCR Detection Kit is capable of detecting *Mycoplasma* infections in cell cultures in less than three hours, depending on the spectrofluorometric thermal cycler used for detection.

Kit Specificity

The *MycoQSearch* Mycoplasma qPCR Detection Kit detects *Mycoplasma* species simply, reliably, and rapidly. To detect the presence of these microorganisms, the assay uses the polymerase chain reaction (PCR) to amplify a target unique to a wide variety of mycoplasmas. The kit can detect more than 50 different *Mycoplasma species*, including *Acholeplasma laidlawii* and *Spiroplasma citri*. The kit does not detect other genera or cell-line DNA.

Kit Sensitivity

The sensitivity of the PCR using this kit is 1 to 10 copies of the target DNA per reaction. Sensitivity of the assay in real culture samples depends on the quality of the sample preparation.

Preventing Template Cross-Contamination

Take precautions to minimize the potential for carryover of nucleic acids from one experiment to the next. Use separate work areas and pipettors for template preparation and PCR setup steps. Use the PCR grade water delivered with the kit, aerosol-preventive filter tips and gloves.

The 2X qPCR master mix contains dUTP instead of dTTP. When dUTP replaces dTTP in PCR amplification, UNG treatment (Uracil-N-glycosylase, not provided in this kit) can prevent the subsequent reamplification of dU-containing PCR products. UNG acts on single- and double-stranded dU-containing DNA by hydrolysis of uracil-glycosidic bonds at dU-containing DNA sites. When this strategy is used, carryover contamination will be eliminated while template DNA (DNA containing T) will be left intact.

Materials Provided

Materials Provided	Quantity		
	QD-Sample	QD-050	QD-100
2X qPCR Master Mix for Probe (Blue Cap)	150µl	750µl	1.5ml
Primer and Probe Mix* (Amber Tube and Cap)	20µl	100µl	200µl
Internal Amplification Control DNA (Orange cap)	20µl	100µl	200µl
Internal Amplification Control DNA for sample prep. (Violet cap)	200µl	1ml	2ml
Positive Control DNA (Yellow Cap)	5µl	25µl	50µl
50X ROX (Reference Dye); High Rox/Low Rox (Amber Tube and Cap)	6µl	30µl	60µl
DNase Free Water (White Cap)	120µl	600µl	1.2ml

*The internal control can be detected with a yellow filter (535–555 nm for Hex). The presence of mycoplasma DNA in the sample is indicated by an increasing fluorescence signal at 510 nm (FAM) and is usually detected with a green filter (470–510 nm).

Storage Conditions

*Upon receipt, store at -20°C. Once thawed, full activity is guaranteed for 6 months.
Repeat thawing reduces quality of product.*

Test Protocol

Prepare the template (Sample)

Samples should be derived from cultures which are at 90-100% confluence. Penicillin and streptomycin in the culture media do not inhibit PCR or affect test sensitivity. To avoid false positive results, we recommend the use of the PCR grade water delivered with the kit, aerosol-preventive filter tips and gloves.

The preparation of sample screening:

Sample preparation from cell culture media

- 1) 1.2 ml liquid supernatant of the sample is transferred into a 1.5ml tube and centrifuged (5 minutes, 1,000 rpm) to sediment cell debris.
- 2) 1ml of the supernatant is transferred into a 1.5ml tube.
- 3) Centrifuged (10 minutes, 13,000 rpm) to sediment mycoplasma particles.
- 4) Discard supernatant and wash the pellet once with 1ml of PBS. Repeat step 3).
- 5) Discard supernatant and add 50µl DNase free water or TE buffer to the pellet.
- 6) Heat the samples at 98°C for 10min, and vortex for 5~10 sec. Then, centrifuge for 5 min at 12,000 rpm with a microcentrifuge. (*Caution!! Be careful when you heat the sample at 98 °C. Heating it in PCR machine with heating cover is recommended.*)
- 7) Transfer the heated supernatant to a fresh tube. This supernatant will be used as the template in the PCR. Take 5µl supernatant as template for qPCR reaction.

*If the template contains PCR inhibition materials, the DNA can be purified with a commercial extraction kit.

The preparation of sample for EP 2.6.7 Guideline:

Genomic DNA extraction

*DNA was isolated using a commercial kit, DNeasy® Blood & Tissue Kit (Cat# 69504, Qia gen, Valencia, CA) following the procedure provided by the vendor

Preparation

All centrifugation steps are carried out at room temperature (15–25°C) in a microcentrifuge. PBS is required for use in step 2. Buffer ATL is not required in this protocol.

Things to do before starting

Buffer AL may form a precipitate upon storage. If necessary, warm to 56°C until the precipitate has fully dissolved.

Buffer AW1 and Buffer AW2 are supplied as concentrates. Before using for the first time, add the appropriate amount of ethanol (96–100%) as indicated on the bottle to obtain a working solution.

Preheat a thermomixer, shaking water bath, or rocking platform to 56°C for use in step 4.

Procedure

- 1) Collect 1ml cell culture (1×10^6 cell/ml) to a tube. Centrifuge for 5 min at 15,000 rpm.**

When using a frozen cell pellet, allow cells to thaw before adding PBS until the pellet can be dislodged by gently flicking the tube.

- 2) Decant the supernatant and resuspend the pellet in 200µl PBS.**
- 3) Add 20µl proteinase K and 20µl Internal Control DNA*. Continue with step 4.**
*The Internal Control DNA for sample prep. of the *MycoQSearch* kit is used to verify the DNA extraction step as well.
- 4) Add 200µl Buffer AL (without added ethanol). Mix thoroughly by vortexing, and incubate at 56°C for 10 min.**
It is essential that the sample and Buffer AL are mixed immediately and thoroughly by vortexing or pipetting to yield a homogeneous solution.
- 5) Add 200µl ethanol (96–100%) to the sample, and mix thoroughly by vortexing.**
It is important that the sample and the ethanol are mixed thoroughly to yield a homogeneous solution.
- 6) Pipet the mixture from step 5 into the DNeasy Mini spin column placed in a 2ml collection tube. Centrifuge at 10,000 rpm for 1 min. Discard flow-through and collection tube.**
- 7) Place the DNeasy Mini spin column in a new 2ml collection tube, add 500µl Buffer AW1, and centrifuge for 1 min 10,000 rpm. Discard flow-through and collection tube.**
- 8) Place the DNeasy Mini spin column in a new 2ml collection tube, add 500µl Buffer AW2, and centrifuge for 1min at 20,000 x g (14,000 rpm).**
- 9) Repeat step 8).**
- 10) Remove the 2ml collection tube solution and centrifuge at 14,000rpm for 3 minutes to dry the column membrane.**

It is important to dry the membrane of the DNeasy Mini spin column, since residual ethanol may interfere with subsequent reactions. This centrifugation step ensures that no residual ethanol will be carried over during the following elution.

Following the centrifugation step, remove the DNeasy Mini spin column carefully so that the column does not come into contact with the flow-through, since this will result in carryover of ethanol. If carryover of ethanol occurs, empty the collection tube, then reuse it in another centrifugation for 1 min at 20,000 x g (14,000 rpm).

- 11) Place the DNeasy Mini spin column in a clean 1.5ml or 2ml microcentrifuge tube, and pipet 100µl Buffer AE directly onto the DNeasy membrane. Incubate at room temperature for 1 min, and then centrifuge for 3 min at 10,000 rpm to elute.**

Prepare for qPCR

1. Prepare the set of reactions listed in the following table. These include two types of control reactions: 1) **positive control** reaction(s) containing Mycoplasma positive control template DNA, and 2) **negative control (no template control)** reaction(s).

Reaction Components	Sample Reaction	Control Reactions	
		Positive Control	NTC (No Template Control)
2X qPCR Master Mix (Blue Cap)	15µl	15µl	15µl
Primer & Probe mix including Internal DNA (Amber Tube and Cap)	2µl	2µl	2µl
Test Sample	5µl	-	-
Internal Amplification Control DNA (Orange cap)	-*	2µl	2µl
Positive Control DNA (Yellow Cap)	-	1 µl	-
50X ROX reference dye** Low ROX / High ROX (Amber tube and Cap)		0µl (No ROX) Low ROX 0.6µl (1X) High ROX 0.6µl (1X)	
DNase Free Water (White Cap)		Up to 30 µl	
Final volume	30µl	30µl	30µl

* In the sample reaction, internal amplification control DNA is not added separately because the sample already include internal amplification control DNA through the sample preparation of DNA extraction procedure.

**ROX concentration for Instruments

Instrument	Reference dye
BioRad: iCycler, MyiQ, MiQ 2, iQ 5, CFX-96, CFX-384, MJ Research: Opticon, Option2, Chromo4, MiniOpticon Qiagen: Roto-Gene Q, Roto-Gene3000, Roto-Gene 6000 Eppendorf: Mastercycler realplex Illumina: Eco RealTime PCR System Roche: LightCycler 480, LightCycler 2.0	No ROX
ABI: 5700, 7000, 7300, 7700, 7900, 7900HT, 7900HT Fast, StepOne, StepOne plus	High ROX(1x)
ABI: 7500, 7500 Fast, QuantStudio (3, 5, 7) Stratagene: MX3000, MX3005P, MX4000	Low ROX(1x)

2. Set up the qPCR instrument to run the PCR cycling (amplification) program specified below.

Steps & Cycle		Temp(°C)	Time
Pre Heat		95	5 min
PCR	45 Cycles	Denature	95 20 sec
		Anneal*	60 30 sec

		Extend	72	30 sec
*Acquisition Mycoplasma DNA - FAM(470~510nm), Green Channel Internal DNA - HEX(535~555), Yellow Channel				

Results


A successfully performed PCR without inhibition is indicated by an increasing fluorescence signal in the internal control channel (HEX). The internal DNA can be detected with a yellow filter (535–555 nm for HEX). The presence of mycoplasma DNA in the sample is indicated by an increasing fluorescence signal at 510 nm (FAM) and is usually detected with a green filter (470–510 nm).

False-negative results (due to inhibition of PCR reaction by the sample matrix) can be detected individually for each sample as these reactions do not show any fluorescence signal.


Using the following table, determine whether the test cell culture is infected with *Mycoplasma*.

<i>FAM Channel (Mycoplasma PCR)</i>	<i>HEX Channel (Internal DNA)</i>	<i>Interpretation</i>
<i>Positive</i>	<i>Positive</i>	<i>Mycoplasma contamination</i>
<i>Negative</i>	<i>Positive</i>	<i>Mycoplasma non-contamination</i>
<i>Negative</i>	<i>Negative</i>	<i>PCR inhibition or Inadequate sample preparation</i>

Internal Control Amplification – HEX (Yellow channel)

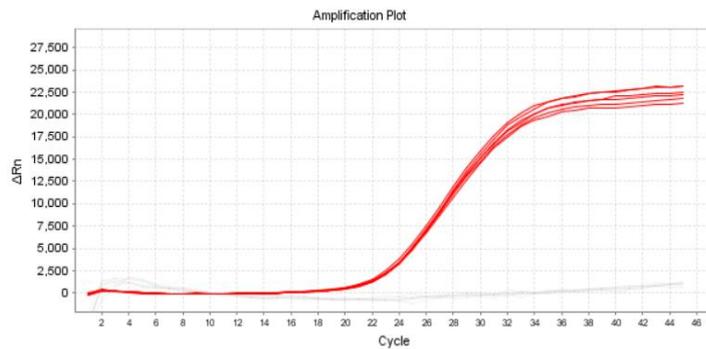

Sample and Positive Control Amplification – FAM (Green channel)

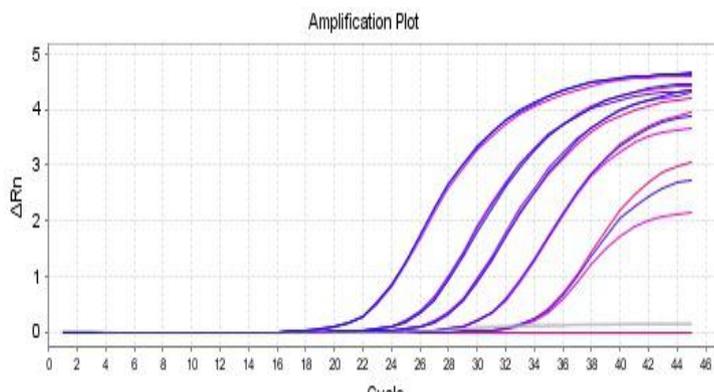

Mycoplasma species detected by *MycoQSearch* Mycoplasma qPCR Detection Kit

1. ****Acholeplasma laidlawii***
2. ****Mycoplasma arginini***
3. ****Mycoplasma fermentans***
4. ****Mycoplasma gallisepticum***
5. ****Mycoplasma hyorhinis***
6. ****Mycoplasma orale***
7. ****Mycoplasma pneumoniae***
8. ****Mycoplasma synoviae***
9. ****Spiroplasma citri***
10. *Mycoplasma agalactica*
11. *Mycoplasma alligatoris*
12. *Mycoplasma anatis*
13. *Mycoplasma arthritidis.*
14. *Mycoplasma bovis*
15. *Mycoplasma bovisgenitalium*
16. *Mycoplasma capricolum*
17. *Mycoplasma cloacale*
18. *Mycoplasma falconis*
19. *Mycoplasma faucium*
20. *Mycoplasma flocculare*
21. *Mycoplasma gallinarum*
22. *Mycoplasma genitalium*
23. *Mycoplasma hominis*
24. *Mycoplasma pneumoniae*
25. *Mycoplasma hyopharyngis*
26. *Mycoplasma hyosynoviae*
27. *Mycoplasma imitans*
28. *Mycoplasma maculosum*
29. *Mycoplasma meleagridis*
30. *Mycoplasma mycoides*
31. *Mycoplasma muris*
32. *Mycoplasma neurolyticum*
33. *Mycoplasma opalescens*
34. *Mycoplasma penetrans*
35. *Mycoplasma pirum*
36. *Mycoplasma primatum*
37. *Mycoplasma pulmonis*
38. *Mycoplasma putrefaciens*
39. *Mycoplasma salivarium strain*
40. *Mycoplasma spermatophilum*
41. *Mycoplasma sp. ovine/caprine*
42. *Mycoplasma sp. putative*
43. *Mycoplasma suis*
44. *Mycoplasma svalvi*
45. *Mycoplasma timone*
46. *Ureaplasma diversum*
47. *Ureaplasma urealyticum*

**Mycoplasma* species in EP 2.6. 7. guidance on the *Mycoplasma* Test